

FIG. 1

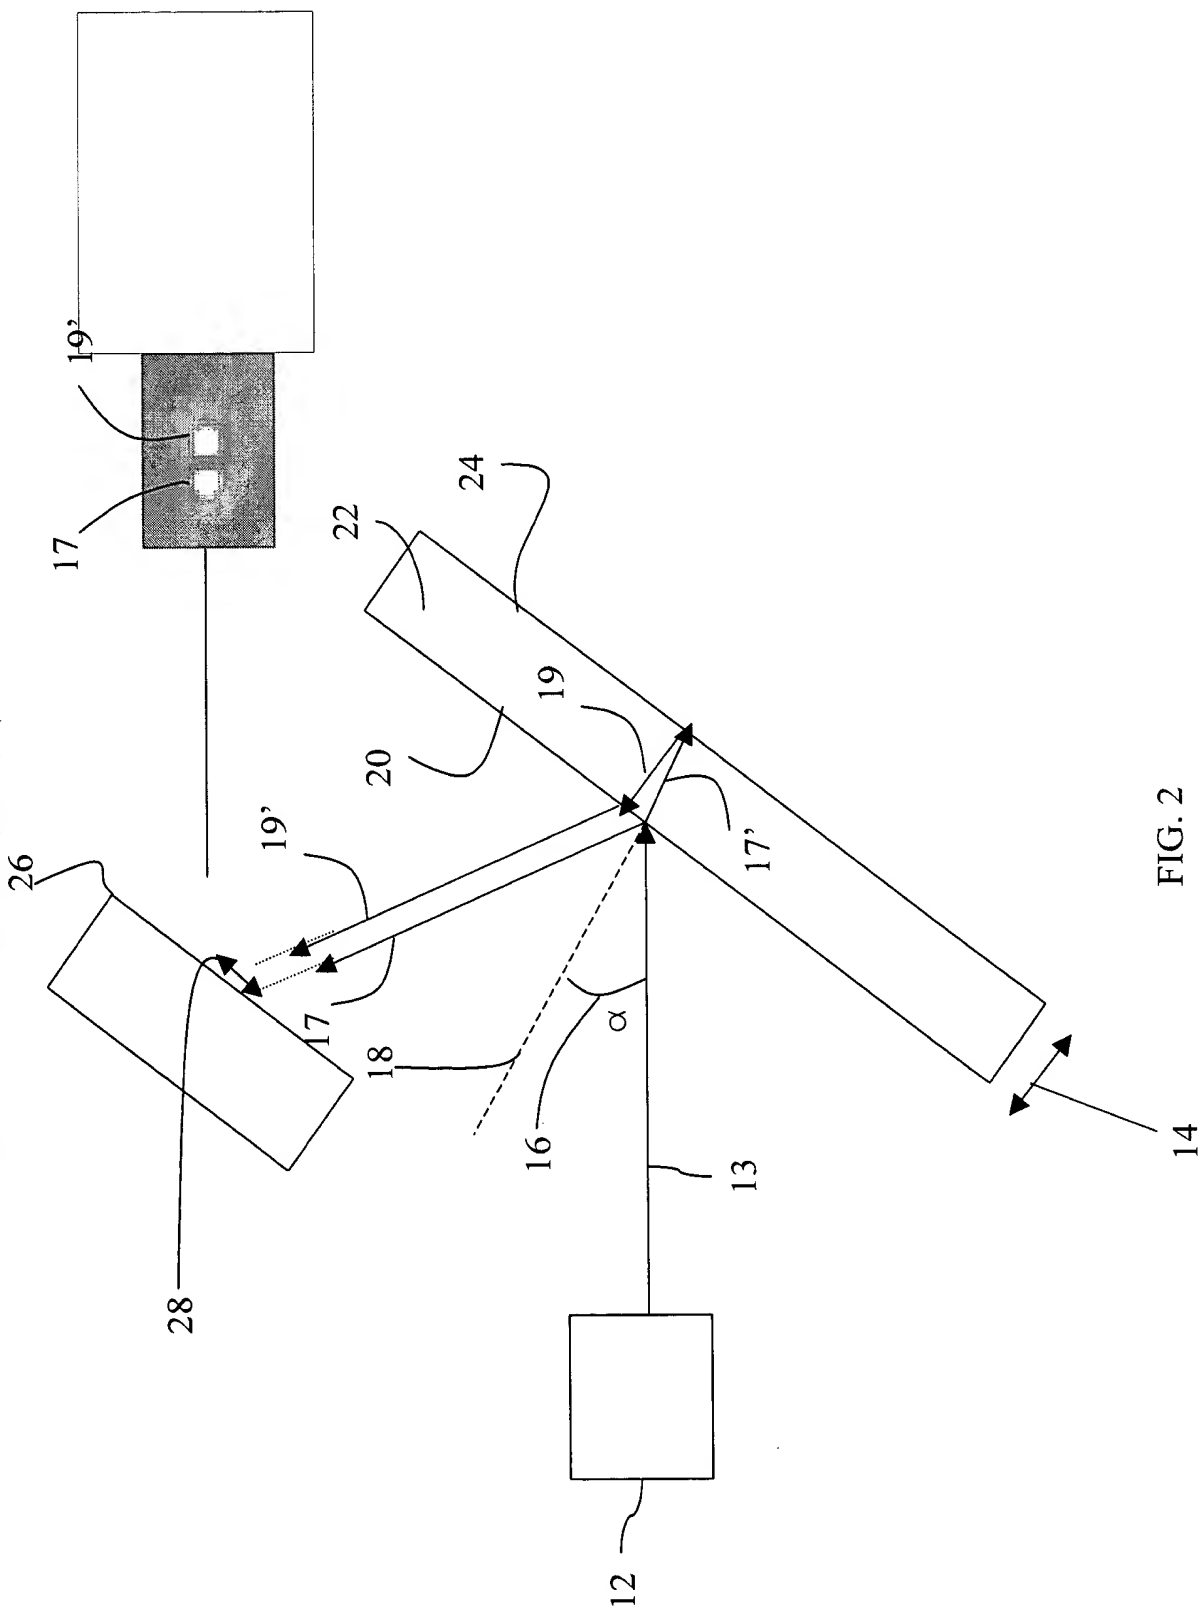


FIG. 2

TOP VIEW OF THE APPARATUS

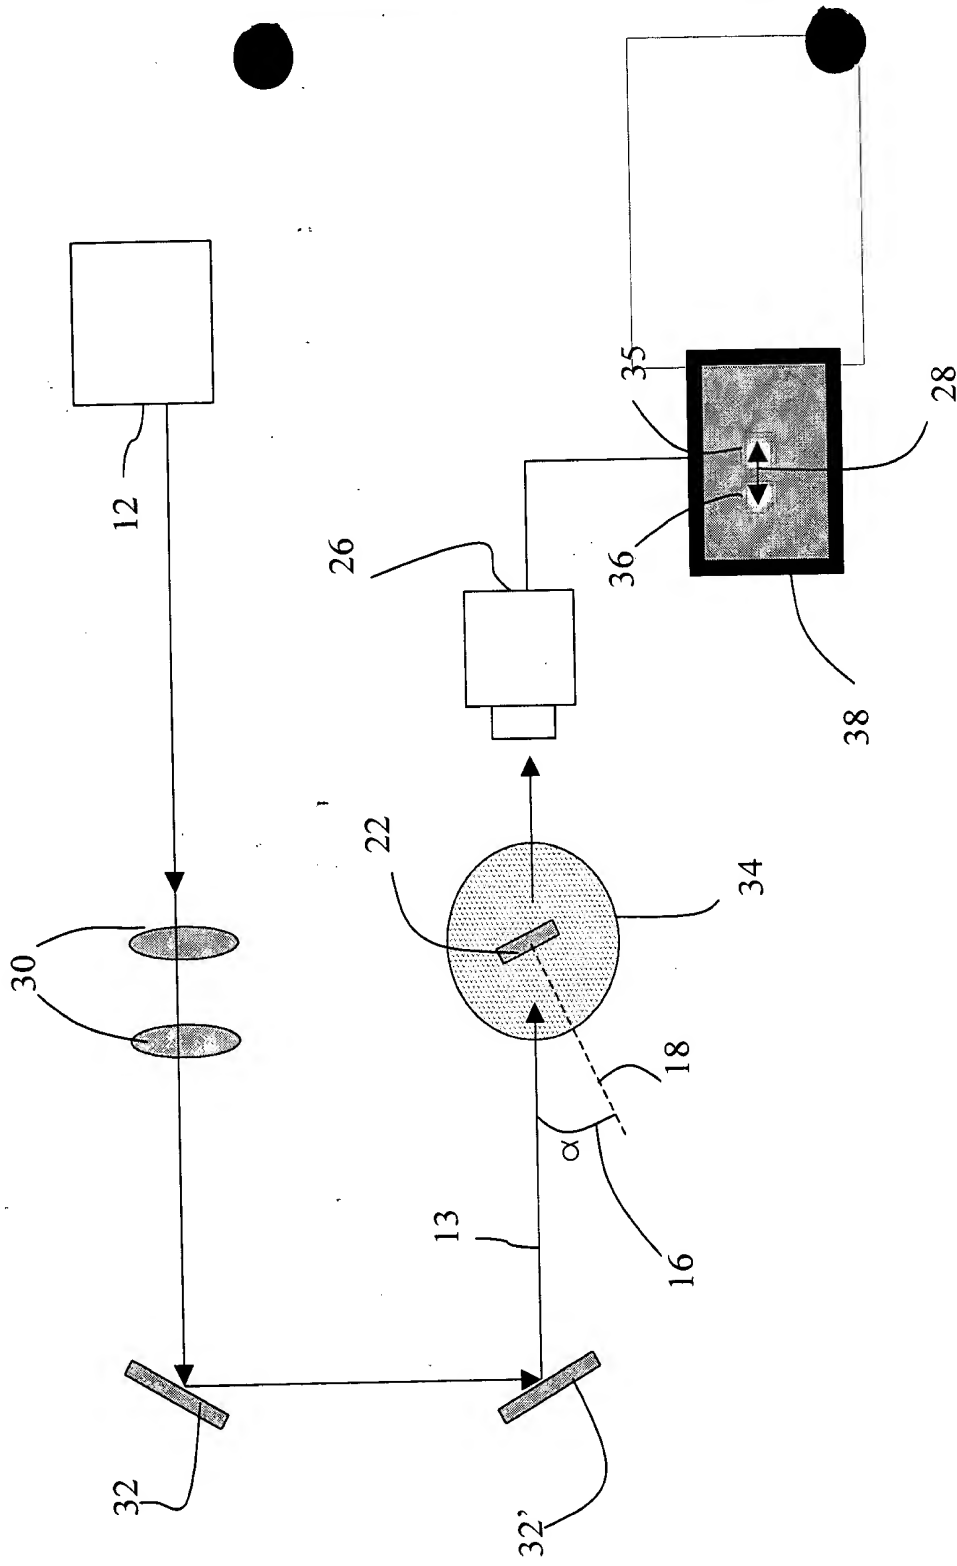


FIG. 3

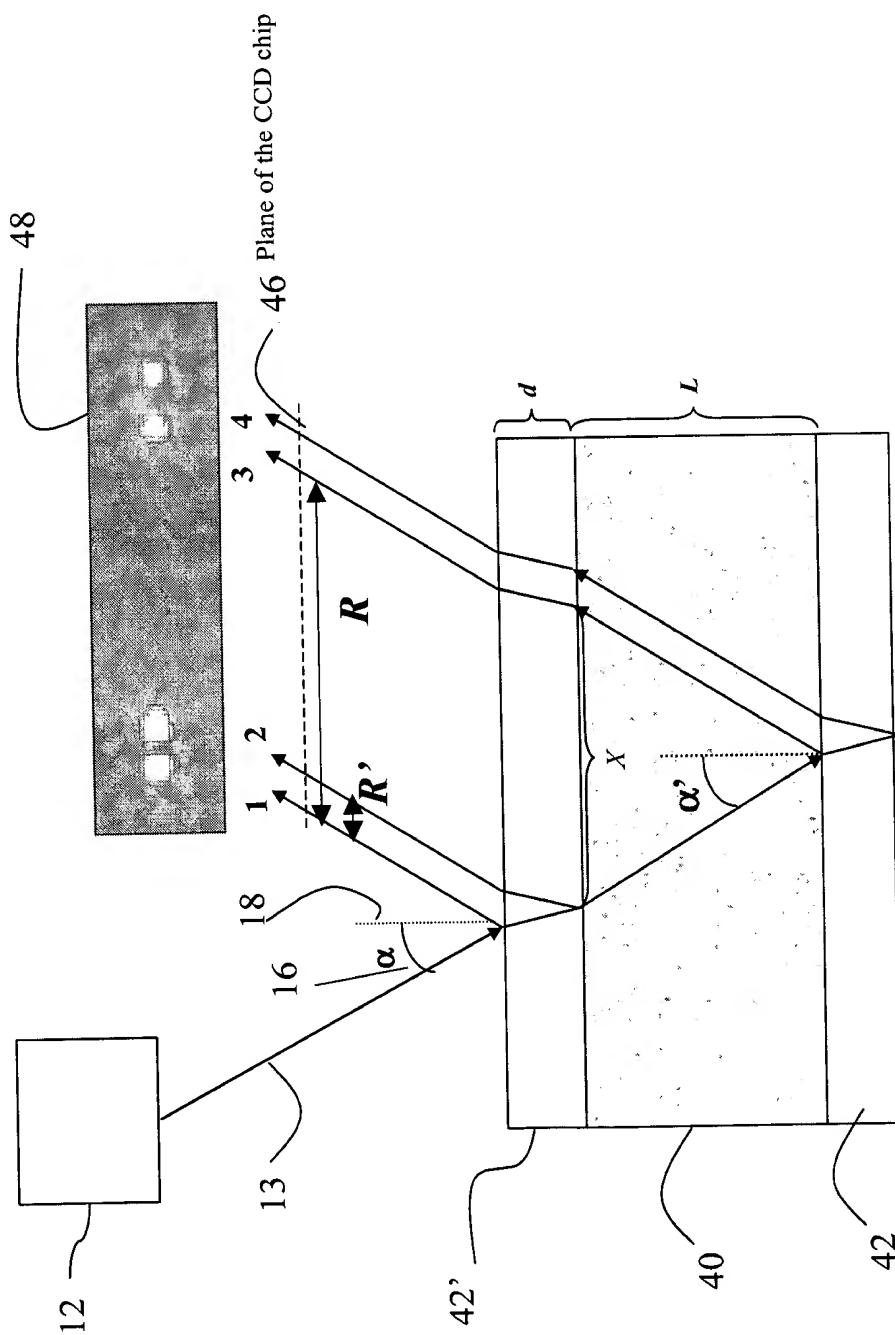


FIG. 4